

State of Nevada Department of Conservation and Natural Resources  
 Division of Environmental Protection  
 Laboratory Scope of Accreditation

**EPA Number: NV00926**


**Attachment to Certificate Number: NV009262019-2**

**Expiration Date: 7/31/2019**

Western Environmental Testing - Elko  
 1084 Lamoille Hwy Elko, NV 89801-

Matrix: **CWA (Non Potable Water)**

Method	Analyte	Start Date	Date Expires	Status
Discipline: Microbiology				
IDEXX Quanti-Tray® using Colilert®	E. coli enumeration	8/1/2018	7/31/2019	Certified
IDEXX Quanti-Tray® using Colilert®-18Hr®	Fecal coliforms	8/1/2018	7/31/2019	Certified

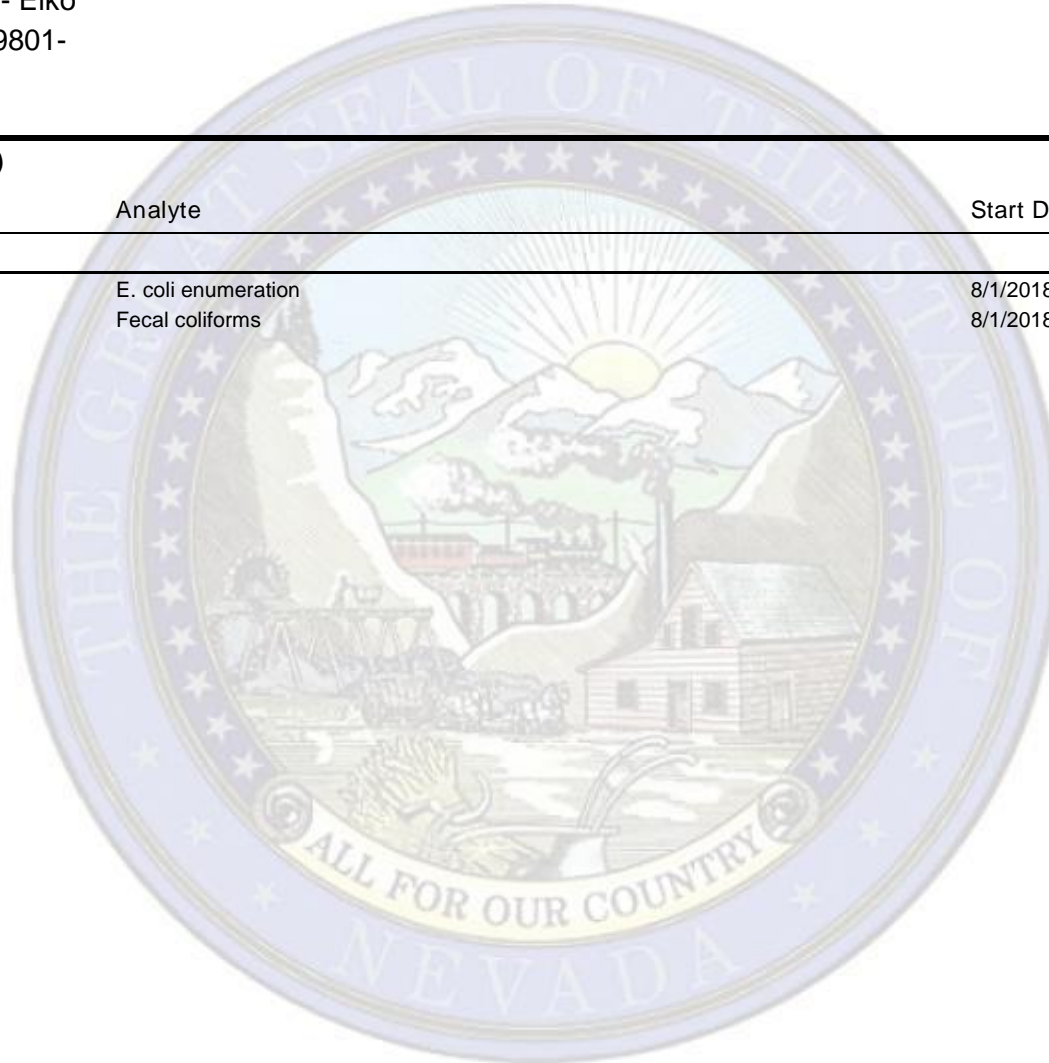

**Disclaimer: A laboratory that is certified or approved has established that they have the ability to implement a quality control program in accordance with the appropriate Federal or State regulations or statutes. It is the certified laboratory's responsibility to provide their client the most current certified parameter list. Contact LCP to verify certification status.**

State of Nevada Department of Conservation and Natural Resources  
 Division of Environmental Protection  
 Laboratory Scope of Accreditation

EPA Number: **NV00926**

Attachment to Certificate Number: **NV009262019-2**

Expiration Date: **7/31/2019**

Western Environmental Testing - Elko  
 1084 Lamoille Hwy Elko, NV 89801-

Matrix: **SDWA (Potable Water)**

Method	Analyte	Start Date	Date Expires	Status
Discipline: Chemistry				
SM 2150 B	Odor	10/2/2018	7/31/2019	Certified
Discipline: Microbiology				
IDEXX Colilert®	Escherichia coli	8/1/2018	7/31/2019	Certified
IDEXX Colilert®	Total coliforms	8/1/2018	7/31/2019	Certified
IDEXX Colilert®-18	Escherichia coli	8/23/2018	7/31/2019	Certified
IDEXX Colilert®-18	Total coliforms	8/23/2018	7/31/2019	Certified
IDEXX Quanti-Tray® under SWTR	E. coli enumeration	8/1/2018	7/31/2019	Certified
IDEXX Quanti-Tray® with Colilert® under SWTR	Total Coliform Enumeration	8/1/2018	7/31/2019	Certified

**Disclaimer:** A laboratory that is certified or approved has established that they have the ability to implement a quality control program in accordance with the appropriate Federal or State regulations or statutes. It is the certified laboratory's responsibility to provide their client the most current certified parameter list. Contact LCP to verify certification status.