

State of Nevada Department of Conservation and Natural Resources
 Division of Environmental Protection
 Laboratory Scope of Accreditation

EPA Number: NV00926


Attachment to Certificate Number: NV009262023-2

Expiration Date: 7/31/2023

Western Environmental Testing - Elko
 1084 Lamoille Hwy Elko, NV 89801-

Matrix: **CWA (Non Potable Water)**

| Method | Analyte | Start Date | Date Expires | Status |
|--|---------------------|------------|--------------|-----------|
| Discipline: Chemistry | | | | |
| SM 2550 B | Temperature, deg. C | 8/1/2022 | 7/31/2023 | Interim |
| Discipline: Microbiology | | | | |
| IDEXX Quanti-Tray® using Colilert®-18Hr® | E. coli enumeration | 8/1/2022 | 7/31/2023 | Certified |
| IDEXX Quanti-Tray® using Colilert®-18Hr® | Fecal coliforms | 8/1/2022 | 7/31/2023 | Certified |

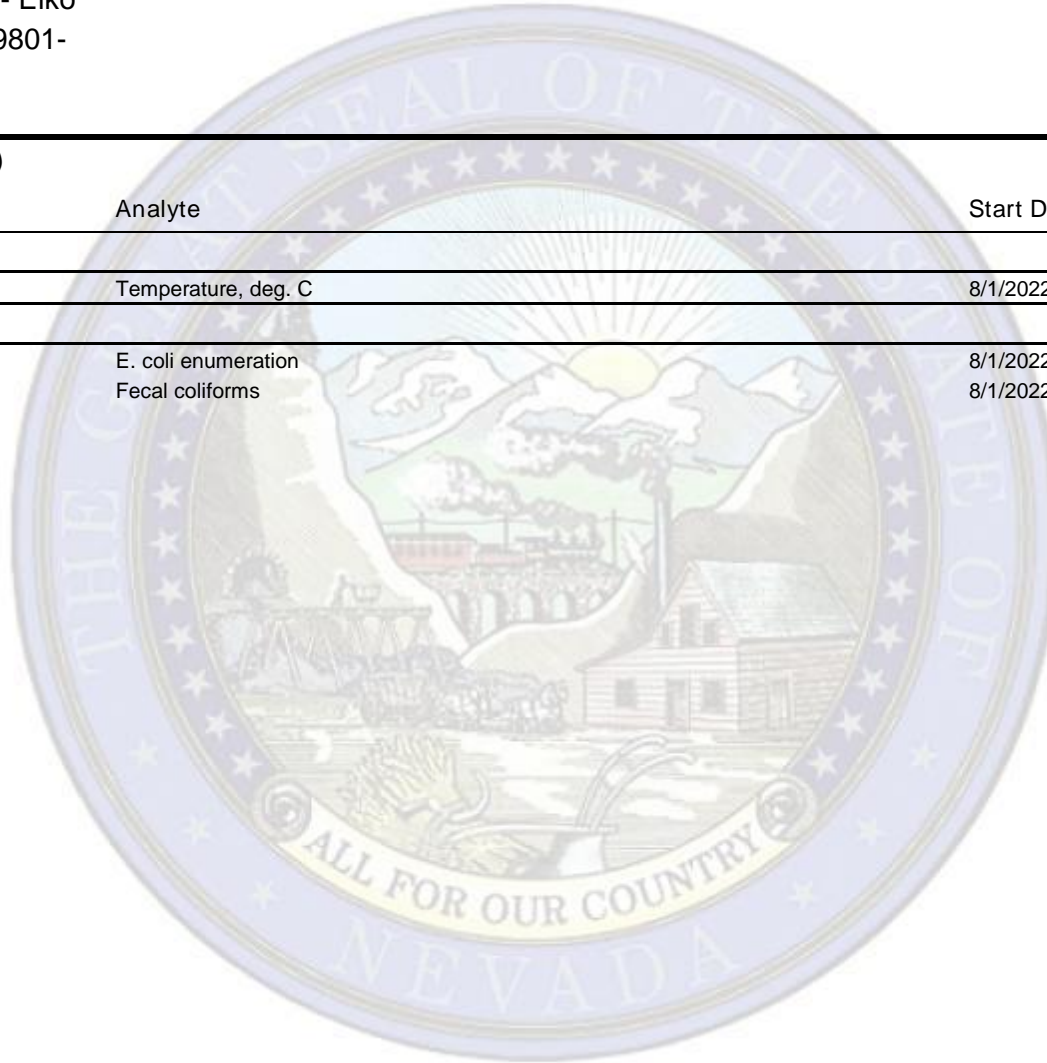

Disclaimer: A laboratory that is certified or approved has established that they have the ability to implement a quality control program in accordance with the appropriate Federal or State regulations or statutes. It is the certified laboratory's responsibility to provide their client the most current certified parameter list. Contact LCP to verify certification status.

State of Nevada Department of Conservation and Natural Resources
 Division of Environmental Protection
 Laboratory Scope of Accreditation

EPA Number: NV00926


Attachment to Certificate Number: NV009262023-2

Expiration Date: 7/31/2023

Western Environmental Testing - Elko
 1084 Lamoille Hwy Elko, NV 89801-

Matrix: **SDWA (Potable Water)**

| Method | Analyte | Start Date | Date Expires | Status |
|---|----------------------------|------------|--------------|-----------|
| Discipline: Chemistry | | | | |
| SM 2150 B | Odor | 8/1/2022 | 7/31/2023 | Certified |
| SM 2550 B | Temperature, deg. C | 8/1/2022 | 7/31/2023 | Interim |
| Discipline: Microbiology | | | | |
| IDEXX Colilert®-18 | Escherichia coli | 8/1/2022 | 7/31/2023 | Certified |
| IDEXX Colilert®-18 | Total coliforms | 8/1/2022 | 7/31/2023 | Certified |
| IDEXX Quanti-Tray® with Colilert®-18 under SWTR | E. coli enumeration | 8/1/2022 | 7/31/2023 | Certified |
| IDEXX Quanti-Tray® with Colilert®-18 under SWTR | Total Coliform Enumeration | 8/1/2022 | 7/31/2023 | Certified |

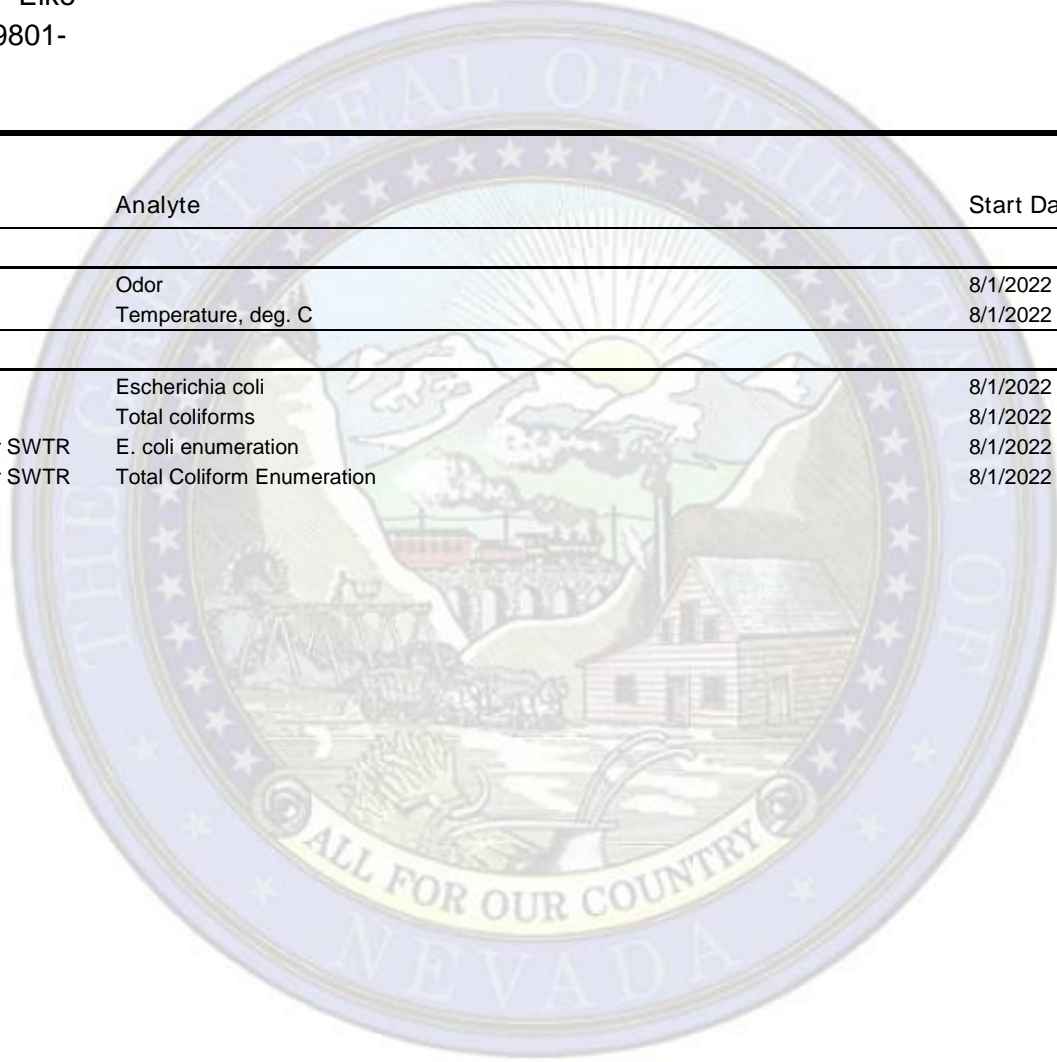

Disclaimer: A laboratory that is certified or approved has established that they have the ability to implement a quality control program in accordance with the appropriate Federal or State regulations or statutes. It is the certified laboratory's responsibility to provide their client the most current certified parameter list. Contact LCP to verify certification status.